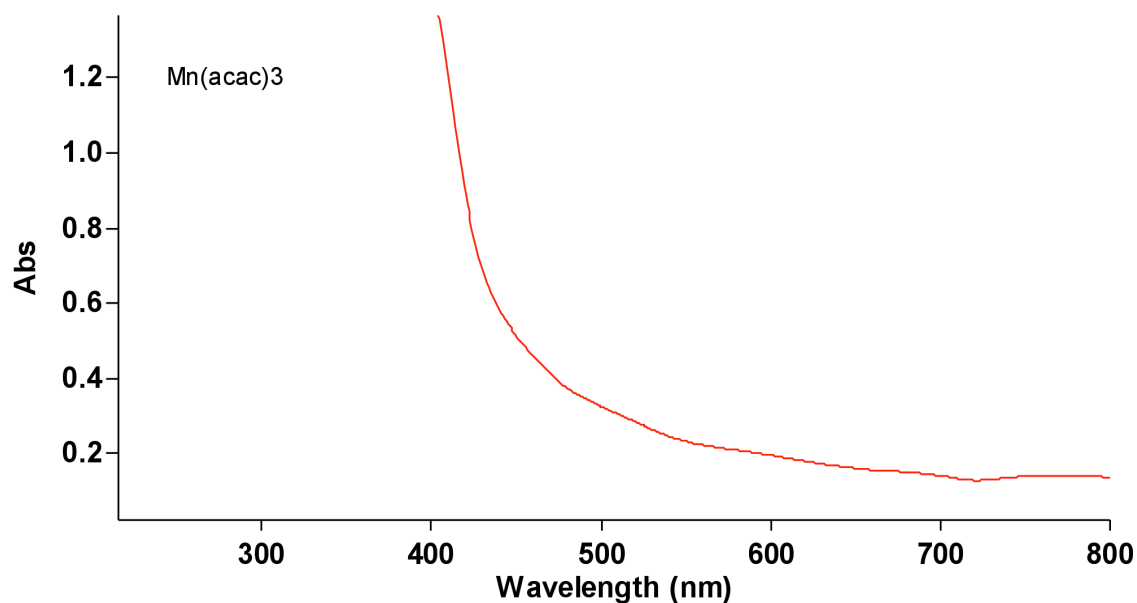


1/5/2021 12:06:28 PM

Page 1 of 2

**Zero Report**

Read Abs (800.0 nm)
Zero 0.0752

Scan Analysis Report

Report Time : Tue 05 Jan 12:04:58 PM 2021
Method
Batch: D:\chem 110\Mnacac3_arj.DSW
Software version: 5.1.0.1016
Operator:

Instrument Parameters

Instrument Cary 60
Instrument Version 2.00
Start (nm) 800.0
Stop (nm) 200.0
X Mode Nanometers
Y Mode Abs
UV-Vis Scan Rate (nm/min) 600.00
UV-Vis Data Interval (nm) 1.00
UV-Vis Ave. Time (sec) 0.1000
Beam Mode Dual Beam
Baseline Correction Off
Cycle Mode Off
Comments

Zero Report

Read Abs (800.0 nm)
Zero 0.0752

Sample Name: sample1

1/5/2021 12:06:28 PM

Page 2 of 2

Collection Time

1/5/2021 12:04:59 PM

Peak Table

Peak Style	Peaks
Peak Threshold	0.0100
Range	800.0nm to 200.0nm
Wavelength (nm)	Abs
353.0	3.787
349.0	4.346
346.0	4.818
343.0	3.926
339.0	4.202
335.0	4.280
333.0	4.830
328.0	10.000
324.0	4.358
321.0	4.075
315.0	4.709
310.0	10.000
306.0	10.000
302.0	4.821
298.0	5.146
295.0	5.125
291.0	4.961
289.0	5.313
286.0	4.519
284.0	4.371
280.0	4.843
277.0	5.027
274.0	5.270
271.0	10.000
266.0	10.000
263.0	10.000
261.0	10.000
256.0	4.492
253.0	5.321
250.0	10.000
246.0	10.000
242.0	4.682
239.0	10.000
237.0	4.717
234.0	10.000
232.0	10.000
229.0	4.964
226.0	4.400
224.0	4.495
222.0	4.362
218.0	4.343
214.0	4.070
211.0	4.262
209.0	4.025
205.0	3.960
202.0	4.221